
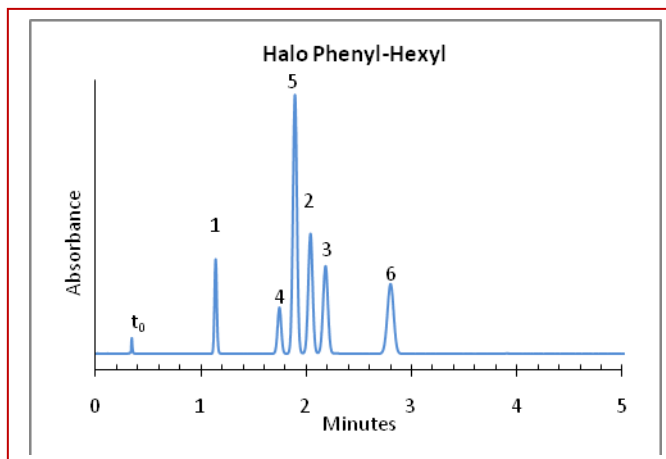


Application Note: 26-P

Separation of Aromatic Nitro compounds on HALO PFP and Phenyl-Hexyl

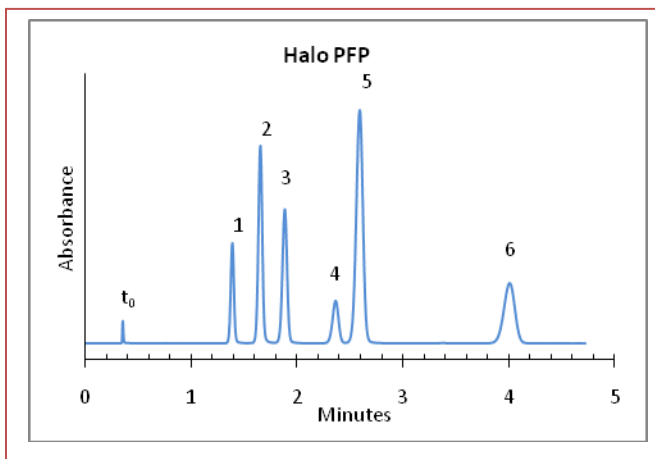


TEST CONDITIONS:

Column: 4.6 x 50 mm, HALO PFP, Phenyl-Hexyl
 Part Numbers: 92814-409, -406, resp.
 Mobile Phase: 45/55-water/methanol
 Flow Rate: 1.5 mL/min.
 Pressure: approximately 200 Bar
 Temperature: 40 °C
 Detection: UV 254 nm, VWD
 Injection Volume: 0.5 µL
 Sample Solvent: ~20/80-water/methanol
 Response Time: 0.02 sec.
 Flow Cell: 2.5 µL semi-micro
 LC System: Shimadzu Prominence UFLC XR
 Extra column volume: ~14 µL


PEAK IDENTITIES:

1. Nitrobenzene
2. 1-Chloro-4-Nitrobenzene
3. 2,6-Dinitrotoluene
4. 4-Nitrotoluene
5. 3-Nitrotoluene
6. 4-Chloro-3-Nitroanisole


STRUCTURES:




Nitrobenzene




1-Chloro-4-Nitrobenzene




2, 6-Dinitrotoluene



4-Nitrotoluene



3-Nitrotoluene



4-Chloro-3-Nitroanisole

Differences in the interaction of the phenyl rings on the bonded phases with the pi electron systems of the nitro aromatic compounds result in significantly different selectivities that can be used to optimize these separations.