


Application Note: 36-EX

## Isocratic Separation of Dinitrotoluenes on HALO PFP Phase

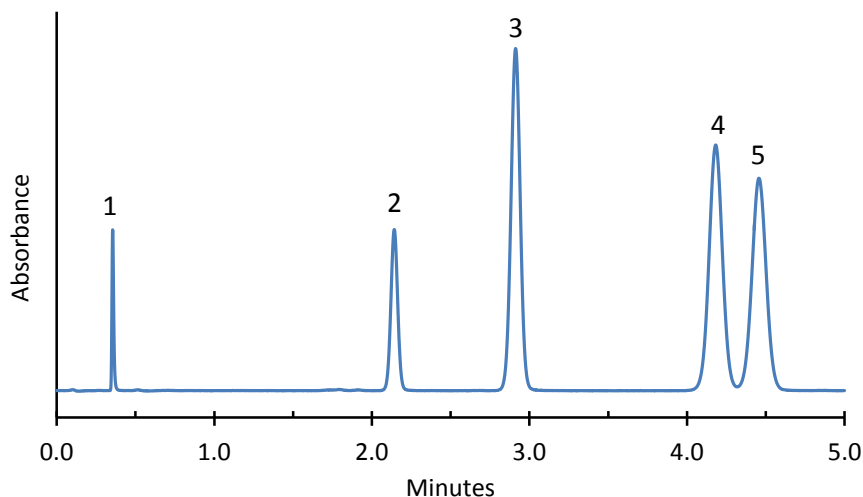


### PEAK IDENTITIES:

1. Uracil
2. 2,6-Dinitrotoluene
3. 2,4-Dinitrotoluene
4. 3,4-Dinitrotoluene
5. 2,3-Dinitrotoluene


### TEST CONDITIONS:

Column: 4.6 x 50 mm, HALO PFP  
 Part Number: 92814-409  
 Mobile Phase: 45/55-Water/Methanol  
 Flow Rate: 1.5 mL/min.  
 Pressure: 225 Bar  
 Temperature: 30 °C  
 Detection: UV 254 nm, VWD  
 Injection Volume: 1.0 µL  
 Sample Solvent: 50/50-Acetonitrile/Methanol  
 Response Time: 0.02 sec.  
 Flow Cell: 2.5 µL semi-micro  
 LC System: Shimadzu Prominence UFLC XR  
 Extra column volume: ~14 µL


### STRUCTURES:




Uracil




3,4-Dinitrotoluene



2,6-Dinitrotoluene



2,3-Dinitrotoluene



2,4-Dinitrotoluene

These dinitrotoluenes are difficult to separate, but can be separated with baseline resolution in under 5 minutes using a HALO Fused Core PFP (perfluorophenylpropyl) column.